

Clontech Laboratories, Inc.

PCR-Select™ cDNA Subtraction Kit User Manual

Cat. No. 637401
(091614)

Clontech Laboratories, Inc.

A Takara Bio Company

1290 Terra Bella Avenue, Mountain View, CA 94043, USA

U.S. Technical Support: tech@clontech.com

United States/Canada	Asia Pacific	Europe	Japan
800.662.2566	+1.650.919.7300	+33.(0)1.3904.6880	+81.(0)77.543.6116

Table of Contents

I. Introduction..... 3

II. List of Components..... 7

III. Additional Materials Required..... 9

IV. PCR-Select cDNA Subtraction Protocols 9

 A. General Considerations 9

 B. RNA Preparation and Handling 10

 C. Protocol: First-Strand cDNA Synthesis 11

 D. Protocol: Second-Strand cDNA Synthesis..... 12

 E. Protocol: Rsa I Digestion 13

 F. Protocol: Adaptor Ligation 14

 G. Protocol: First Hybridization 17

 H. Protocol: Second Hybridization 17

 I. Protocol: PCR Amplification..... 18

V. Analysis of Results & Troubleshooting Guide 21

 A. Analysis of ds cDNA Synthesis Products 21

 B. Analysis of Rsa I Digestion 21

 C. Analysis of Ligation..... 22

 D. Analysis of PCR Products..... 24

 E. PCR Analysis of Subtraction Efficiency..... 26

 F. Hybridization Analysis of Subtraction Efficiency 28

VI. Differential Screening of the Subtracted Library..... 30

VII. References..... 31

Appendix A: Suppression PCR..... 34

Appendix B: Adaptor and Primer Sequences..... 35

Table of Figures

Figure 1. Overview of the PCR-Select procedure..... 5

Figure 2. Schematic diagram of PCR-Select cDNA subtraction.. 6

Figure 3. Preparing adaptor-ligated tester cDNAs for hybridization and PCR..... 14

Figure 4. Positive control skeletal muscle ds cDNA before (Lane 1) and after (Lane 2) Rsa I digestion. 21

Figure 5. Typical results of ligation efficiency analysis.. 24

Figure 6. Typical results of control skeletal muscle subtraction analysis. 25

Figure 7. Reduction of G3PDH abundance by PCR-Select subtraction. 27

Figure 8. Enrichment of a differentially expressed gene and reduction of an abundant housekeeping gene in Jurkat cells. 28

Figure 9. Southern blot analysis of PCR-Select subtraction. 29

Figure 10. Suppression PCR. 34

Figure 11. Sequences of the PCR-Select cDNA synthesis primer, adaptors, PCR primers, and Control Primers. 35

Table of Tables

Table 1. Setting up the Ligation Reactions	16
Table 2. Setting Up the First Hybridization.....	17
Table 3. Preparation of the Primary PCR Master Mix.....	19
Table 4. Preparation of the Secondary PCR Master Mix.....	20
Table 5. Setting Up the Ligation Analysis.....	22
Table 6. Preparation of the Ligation Analysis PCR Master Mix	22

I. Introduction

A. Summary

Subtractive hybridization is a powerful technique that enables researchers to compare two populations of mRNA and obtain clones of genes that are expressed in one population but not in the other. Although there are several different methods, the basic theory behind subtraction is simple. First, both mRNA populations are converted into cDNA: we refer to the cDNA that contains specific (differentially expressed) transcripts as **tester**, and the reference cDNA as **driver**. Tester and driver cDNAs are hybridized, and the hybrid sequences are then removed. Consequently, the remaining unhybridized cDNAs represent genes that are expressed in the tester yet absent from the driver mRNA.

The **PCR-Select cDNA Subtraction Kit** is based on a unique method of selective amplification of differentially expressed sequences, which overcomes the technical limitations of traditional subtraction methods (Diatchenko *et al.*, 1996; Gurskaya *et al.*, 1996). Figure 1 presents a brief overview of the PCR-Select procedure.

B. Molecular Basis of PCR-Select cDNA Subtraction

The following molecular events (Figures 1 & 2) occur during PCR-Select cDNA subtraction:

1. **cDNA synthesis (Sections IV.C & IV.D)**

The tester and driver cDNAs are synthesized from poly A⁺ RNA generated from the two types of tissues or cells being compared.

2. **Restriction digestion to make cDNA ends blunt (Section IV.E)**

The tester and driver cDNAs are each digested with a restriction enzyme such as Rsa I (supplied with this kit) to yield shorter, blunt-ended molecules.

3. **Adaptor ligation (Section IV.F)**

The tester cDNA is then subdivided into two portions, and each is ligated with a different cDNA adaptor. The ends of the adaptor do not contain a phosphate group, so only one strand of each adaptor attaches to the 5' ends of the cDNA. The two adaptors have stretches of identical sequence to allow annealing of the PCR primer once the recessed ends have been filled in. (See Appendix B for detailed sequences of the primers and adaptors).

4. First hybridization (Section IV.G)

The first of two successive hybridizations is performed in order to equalize and enrich differentially expressed sequences:

- An excess of driver is added to each sample of tester. The samples are then heat denatured and allowed to anneal, generating the type **a**, **b**, **c**, and **d** molecules in each sample (Figure 2).
- The concentration of high- and low-abundance sequences is equalized among the type **a** molecules because reannealing is faster for the more abundant molecules due to the second-order kinetics of hybridization. At the same time, type **a** molecules are significantly enriched for differentially expressed sequences while cDNAs that are not differentially expressed form type **c** molecules with the driver.

5. Second hybridization (Section IV.H)

The two primary hybridization samples are mixed together without denaturing in order to generate PCR templates from differentially expressed sequences:

- Only the remaining equalized and subtracted ss tester cDNAs can reassociate and form new type **e** hybrids. These new hybrids are ds tester molecules with different ends, which correspond to the sequences of Adaptors 1 and 2R.
- Fresh denatured driver cDNA is added (again, without denaturing the subtraction mix) to further enrich fraction **e** for differentially expressed sequences. After filling in the ends by DNA polymerase, the type **e** molecules—the differentially expressed tester sequences—have different annealing sites for the nested primers on their 5' and 3' ends.

6. First PCR amplification (Section IV.I)

The entire population of molecules is then subjected to suppression PCR, which exponentially amplifies only the desired differentially expressed sequences.

- During this PCR, type **a** and **d** molecules are missing primer annealing sites, and thus cannot be amplified.
- Due to the suppression PCR effect, most type **b** molecules form a pan-like structure that prevents their exponential amplification (see Appendix A for more details.)
- Type **c** molecules have only one primer annealing site and amplify linearly.
- Only type **e** molecules—the equalized, differentially expressed sequences with two different adaptors—amplify exponentially.

7. Second PCR amplification (Section IV.I)

A secondary PCR amplification is performed using nested primers to further reduce any background PCR products and enrich for differentially expressed sequences.

8. Clone and confirm differentially expressed genes

The cDNAs can then be cloned, allowing identification of differentially expressed RNAs by sequence and/or hybridization analysis. Additionally, the PCR mixture can be used as a hybridization probe to screen DNA libraries. The **Clontech PCR-Select Differential Screening Kit** (Cat. No. 637403) can be used to quickly confirm that individual clones represent differentially expressed genes.

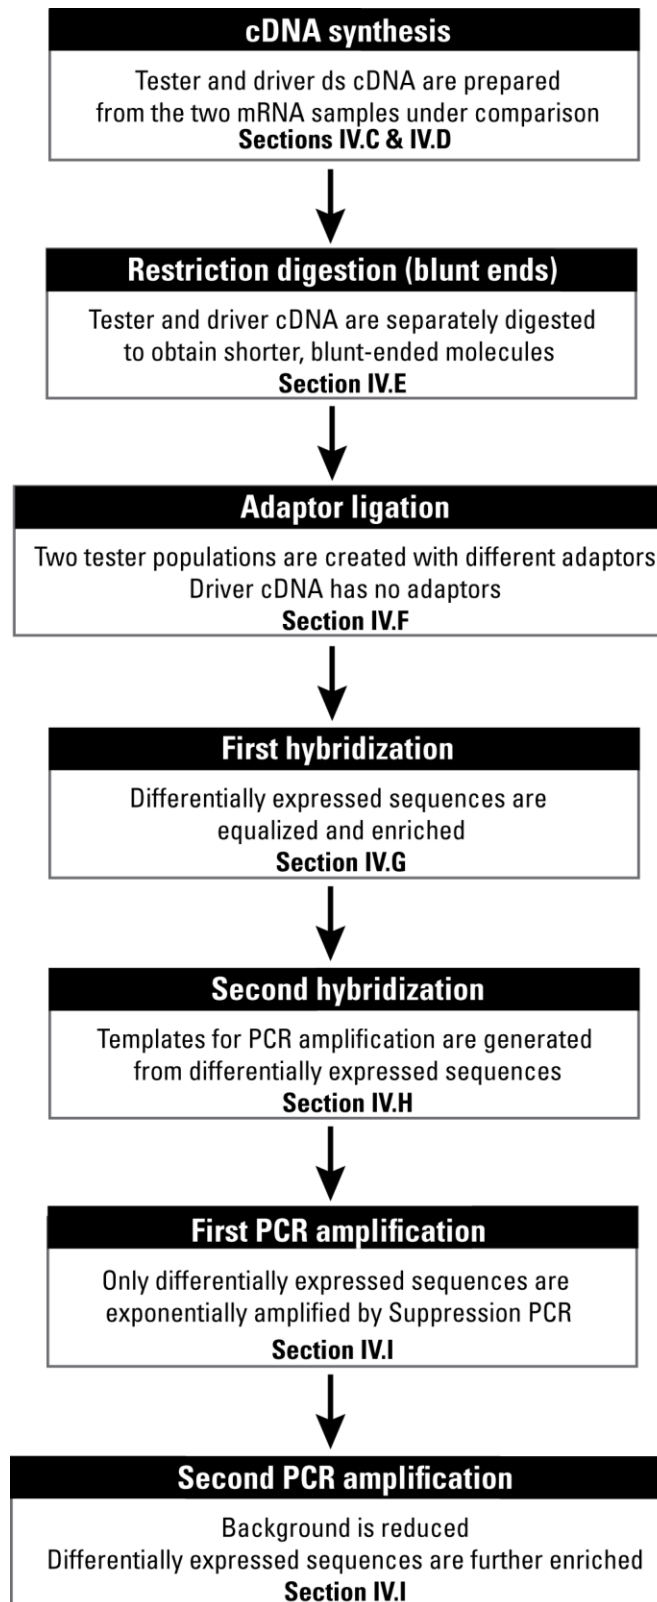


Figure 1. Overview of the PCR-Select procedure. The cDNA in which specific transcripts are to be found is referred to as tester and the reference cDNA is referred to as driver. If you use the SMARTer™ Pico PCR cDNA Synthesis Kit (Cat. No. 634928) for cDNA synthesis, you should begin with the adaptor ligation step (Section IV.F) shown above.

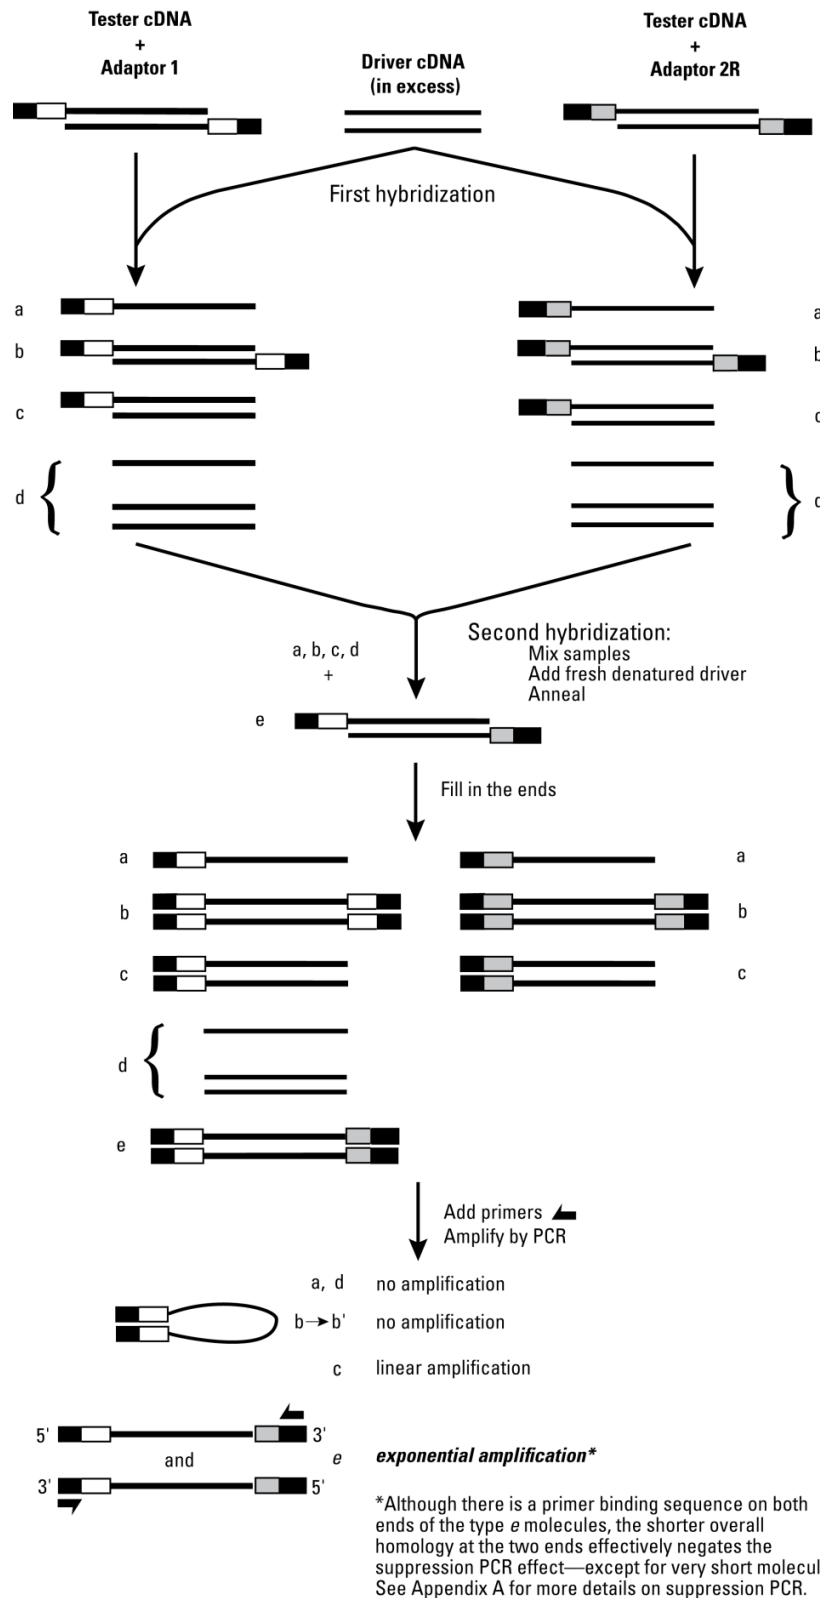


Figure 2. Schematic diagram of PCR-Select cDNA subtraction. Type e molecules are formed only if the sequence is upregulated in the tester cDNA. Solid lines represent the Rsa I-digested tester or driver cDNA. Solid boxes represent the outer part of the Adaptor 1 and 2R longer strands and corresponding PCR primer 1 sequence. Clear boxes represent the inner part of Adaptor 1 and the corresponding Nested PCR primer 1 sequence. Shaded boxes represent the inner part of Adaptor 2R and the corresponding Nested PCR primer 2R sequence.

II. List of Components

Store RNA at -70°C . Store all other reagents at -20°C .

This kit includes enough reagents for seven cDNA syntheses:

- For best results, use 2 μg of poly A⁺ RNA per reaction; differentially expressed cDNAs for rare transcripts may be lost during subtraction if less poly A⁺ RNA is used.
- The seven cDNA syntheses are equivalent to six complete subtraction experiments and one control, assuming the cDNA from each synthesis is used for tester and driver in separate experiments (for identifying up- and down-regulated cDNAs in a particular system).
- Enough PCR reagents are provided for 50 primary and 100 secondary PCRs. Refer to Appendix B for detailed adaptor and primer sequences.

First-Strand Synthesis

- 7 μl SMARTScribe™ Reverse Transcriptase (100 units/ μl)
- 10 μl cDNA Synthesis Primer (10 μM)
- 200 μl 5X First-Strand Buffer (RNase-free)
 - 250 mM Tris-HCl (pH 8.3)
 - 30 mM MgCl₂
 - 375 mM KCl
- 10 μl Dithiothreitol (DTT; 20 mM)

Second-Strand Synthesis

- 28 μl 20X Second-Strand Enzyme Cocktail
 - DNA polymerase I, 6 units/ μl
 - RNase H, 0.25 units/ μl
 - E. coli* DNA ligase, 1.2 units/ μl
- 200 μl 5X Second-Strand Buffer
 - 500 mM KCl
 - 50 mM Ammonium sulfate
 - 25 mM MgCl₂
 - 0.75 mM β -NAD
 - 100 mM Tris-HCl (pH 7.5)
 - 0.25 mM BSA
- 14 μl T4 DNA Polymerase (3 units/ μl)

Endonuclease Digestion

- 300 μl 10X Rsa I Restriction Buffer
 - 100 mM Bis Tris Propane-HCl (pH 7.0)
 - 100 mM MgCl₂
 - 1 mM DTT
- 12 μl Rsa I (10 units/ μl)

Adaptor Ligation

- 21 µl T4 DNA Ligase (400 units/µl; contains 3 mM ATP)
- 200 µl 5X DNA Ligation Buffer
 - 250 mM Tris-HCl (pH 7.8)
 - 50 mM MgCl₂
 - 10 mM DTT
 - 0.25 mM BSA
- 30 µl Adaptor 1 (10 µM)
- 30 µl Adaptor 2R (10 µM)

Hybridization

- 200 µl 4X Hybridization Buffer
- 1.4 ml Dilution buffer
 - 20 mM HEPES (pH 8.3)
 - 50 mM NaCl
 - 0.2 mM EDTA (pH 8.0)

PCR Amplification

- 50 µl PCR Primer 1 (10 µM)
- 100 µl Nested PCR primer 1 (10 µM)
- 100 µl Nested PCR primer 2R (10 µM)
- 10 µl PCR Control Subtracted cDNA

Control Reagents

- 5 µl Control Poly A⁺ RNA (1 µg/µl; from human skeletal muscle)
- 5 µl Control DNA (3 ng/µl; Hae III-digested bacteriophage φX174 DNA)
- 50 µl G3PDH 5' Primer (10 µM)*
- 50 µl G3PDH 3' Primer (10 µM)*

* These primers will amplify human, mouse, and rat G3PDH genes.

General Reagents

- 20 µl dNTP Mix (10 mM each dATP, dCTP, dGTP, dTTP)
- 100 µl 20X EDTA/glycogen Mix (0.2 M EDTA; 1 mg/ml glycogen)
- 480 µl NH₄OAc (4 M)
- 1 ml sterile H₂O

III. Additional Materials Required

The following reagents are required but not supplied.

- **Hae III digest of bacteriophage ϕ X174**
We recommend Takara Bio DNA size markers (Cat. Nos. 3405A & 3405B)
- **0.5 ml PCR reaction tubes**
We recommend GeneAmp 0.5 ml reaction tubes (Applied Biosystems, Cat. Nos. N8010737 or N8010180).
- **80% ethanol & 96% ethanol**
- **Phenol:chloroform:isoamyl alcohol (25:24:1)**
- **Chloroform:isoamyl alcohol (24:1)**
- **50X PCR enzyme mix**
We recommend our Advantage® cDNA Polymerase Mix (Cat. No. 639105), which is also provided in the Advantage cDNA PCR Kits (Cat. Nos. 639101 & 639102).
- **10X PCR buffer**
Use the 10X reaction buffer supplied with your DNA polymerase or mix (included with Advantage cDNA Polymerase Mix (Cat. No. 639105) and the Advantage cDNA PCR Kits (Cat. Nos. 639101 & 639102).
- **dNTP Mix for PCR** (10 mM each dATP, dCTP, dGTP, dTTP)
- **50X TAE electrophoresis buffer**

242 g	Tris base
57.1 ml	Glacial acetic acid
37.2 g	Na ₂ EDTA•H ₂ O

Add H₂O to 1 L. For 1X TAE buffer, dilute 50X stock solution 1:49 with H₂O.

IV. PCR-Select cDNA Subtraction Protocols

PLEASE READ ENTIRE PROTOCOL BEFORE STARTING.

A. General Considerations

- Wear gloves to protect RNA and cDNA samples from degradation by nucleases.
- If you use the PCR-Select Differential Screening Kit (Cat. No. 637403) to differentially screen your samples before performing Northern blot analysis, you will need to perform two subtractions: your original intended subtraction (forward subtraction), and a reverse subtraction, in which tester serves as driver and driver as tester. For more information about differential screening, see Section VI and the PCR-Select Differential Screening Kit User Manual at www.clontech.com/manuals
- A hot start **MUST** be used to reduce nonspecific DNA synthesis during the setup of the PCR. We recommend using either TaqStart® Antibody (Kellogg *et al.*, 1994) or manual hot start (D'Aquila *et al.*, 1991). This protocol was optimized using our TaqStart Antibody (individually available as Cat. Nos. 639250 & 639251; also included in our Advantage cDNA Polymerase Mix (Cat. No. 639105).
- Do not increase the amount of enzyme or concentration of DNA in the reactions as these have been carefully optimized.

B. RNA Preparation and Handling

1. General precautions

Intact, pure poly A⁺ RNA is essential for the synthesis of high-quality cDNA. To avoid RNA contamination and degradation, as well as minimize the presence of RNases, use the following precautions:

- Wear gloves to prevent RNase contamination from your hands
- Use aerosol-free pipette tips for dispensing small volumes (or sterile disposable pipettes for larger volumes).

2. RNA isolation

- See Farrell *et al.*, 1993 or Sambrook *et al.*, 2001 for procedures.
- Whenever possible, the total RNA samples being compared should be purified side-by-side using the same reagents and protocol. This practice reduces the likelihood of false positives.

3. RNA analysis

After total and poly A⁺ RNA isolation, examine RNA integrity by electrophoresing samples on a denaturing, formaldehyde 1% agarose/EtBr gel. Analyze results according to the following criteria:

- **Intact total mammalian RNA** typically exhibits two bright bands—corresponding to ribosomal 28S and 18S RNA—at ~4.5 and 1.9 kb, respectively, with a ratio of intensities of ~1.5–2.5:1.
- **Mammalian poly A⁺ RNA** appears as a smear from 0.5–12 kb with weak ribosomal RNA bands present. The size distribution may be smaller (0.5–3 kb) for nonmammalian species.
- **If your experimental RNA appears smaller than expected** (e.g., no larger than 1–2 kb), as a smear <1–2 kb, and/or the ratio of intensity of 28S to 18S observed is <1:1, your RNA may have been impure or degraded.
 - We suggest you test all RNA isolation reagents for the presence of RNase or other impurities. If contamination is found, you must prepare RNA again using fresh reagents if necessary.
 - If problems persist, you may need to identify another source of tissue or cells, such as our Premium Poly A⁺ RNAs. Poor quality and/or degraded RNA produces high background in the subtraction procedure and should not be used as starting material.

C. Protocol: First-Strand cDNA Synthesis

Perform this procedure with each experimental tester and driver poly A⁺ RNA, and with the Control Poly A⁺ RNA (from human skeletal muscle) provided with the kit.

General Considerations Regarding Controls

- The skeletal muscle cDNA made in this section serves as control driver cDNA in later steps.
- In Section IV.F.2, mock tester cDNA is generated by adding a small amount of the Control DNA (Hae III-digested φX174) to an aliquot of the skeletal muscle ds cDNA.
- You should then perform a complete control subtraction with these skeletal muscle tester and driver cDNAs in parallel with your experimental subtraction. The control subtraction allows you to estimate both the yield and size distribution of synthesized ds cDNA.

Procedure for First-Strand cDNA Synthesis

1. For each tester, driver, and the Control Poly A⁺ RNA (from human skeletal muscle), combine the following components in a sterile 0.5 ml microcentrifuge tube. (Do not use a polystyrene tube).

	<u>per rxn</u>
Poly A ⁺ RNA (2 µg)	2–3 µl*
cDNA Synthesis Primer (10 µM)	1 µl

*For the control synthesis, add 2 µl of the skeletal muscle control poly A⁺ RNA.

If needed, add sterile H₂O to a final volume of 4 µl. Mix contents and spin briefly in a microcentrifuge.

2. Incubate at 70°C for 2 min in a thermal cycler.
3. Cool on ice for 2 min and briefly centrifuge.
4. Add the following reagents to each reaction:

	<u>per rxn</u>
5X First-Strand Buffer	2 µl
dNTP Mix (10 mM each)	1 µl
Sterile H ₂ O	1 µl
DTT (20 mM)	1 µl
SMARTScribe Reverse Transcriptase (100 units/µl)	1 µl

5. Gently vortex and briefly centrifuge the tubes.
6. Incubate the tubes at 42°C for 1.5 hr in an air incubator.

NOTE: Do not use a water bath or thermal cycler. Evaporation can reduce the reaction mixture volume, and therefore, reaction efficiency.

7. Place on ice to terminate first-strand cDNA synthesis and immediately proceed to Section IV.D.

D. Protocol: Second-Strand cDNA Synthesis

Perform the following procedure with each first-strand tester, driver, and the control skeletal muscle cDNA.

1. Add the following components to the first-strand synthesis reaction tubes (containing 10 µl):

	per rxn
Sterile H ₂ O	48.4 µl
5X Second-Strand Buffer	16.0 µl
dNTP Mix (10 mM)	1.6 µl
20X Second-Strand Enzyme Cocktail	4.0 µl

2. Mix contents and briefly spin. The final volume should be 80 µl.
3. Incubate at 16°C for 2 hr in water bath or thermal cycler.
4. Add 2 µl (6 u) of T4 DNA Polymerase. Mix contents well.
5. Incubate at 16°C for 30 min in a water bath or thermal cycler.
6. Add 4 µl of 20X EDTA/Glycogen Mix to terminate second-strand synthesis.
7. Add 100 µl of phenol:chloroform:isoamyl alcohol (25:24:1).
8. Vortex thoroughly, and centrifuge at 14,000 rpm for 10 min at room temperature to separate phases.
9. Carefully collect the top aqueous layer and place in a fresh 0.5 ml microcentrifuge tube. Discard the inter- and lower phases and dispose of them appropriately.
10. Add 100 µl of chloroform:isoamyl alcohol (24:1).
11. Repeat Steps 8 and 9.
12. Add 40 µl of 4 M NH₄OAc and 300 µl of 95% ethanol.

NOTE: Proceed immediately with precipitation. **Do not** store tubes at -20°C. Prolonged exposure to this temperature can precipitate undesired salts.

13. Vortex thoroughly and centrifuge at 14,000 rpm for 20 min at room temperature.
14. Carefully collect the supernatant.
15. Overlay the pellet with 500 µl of 80% ethanol.
16. Centrifuge at 14,000 rpm for 10 min.
17. Remove the supernatant.
18. Air dry the pellet for about 10 min to evaporate residual ethanol.
19. Dissolve precipitate in 50 µl of sterile H₂O.
20. Transfer 6 µl to a fresh microcentrifuge tube. Store this sample at -20°C until after Rsa I digestion (for agarose gel electrophoresis) to estimate yield and size range of ds cDNA products synthesized (see Section V.A)

E. Protocol: Rsa I Digestion

Perform the following procedure with each experimental ds tester and driver cDNA, as well as with the control skeletal muscle cDNA. This step generates shorter, blunt-ended ds cDNA fragments which are optimal for subtraction and required for adaptor ligation in Section IV.F.

1. Add the following reagents to each reaction:

	per rxn
ds cDNA	43.5 µl
10X Rsa I Restriction Buffer	5.0 µl
Rsa I (10 units/µl)	1.5 µl

2. Mix by vortexing and briefly centrifuge.
3. Incubate at 37°C for 1.5 hr.
4. Set aside 5 µl of the digest mixture to analyze the efficiency of Rsa I digestion as described in Section V.B.
5. Add 2.5 µl of 20X EDTA/Glycogen Mix to terminate the reaction.
6. Add 50 µl of phenol:chloroform:isoamyl alcohol (25:24:1).
7. Vortex thoroughly and centrifuge at 14,000 rpm for 10 min at room temperature to separate phases.
8. Carefully collect the top aqueous layer and place in a fresh 0.5 ml tube.
9. Add 50 µl of chloroform:isoamyl alcohol (24:1).
10. Repeat steps 7 and 8.
11. Add 25 µl of 4 M NH₄OAc and 187.5 µl of 95% ethanol.

NOTE: Proceed immediately with precipitation. **Do not** store tubes at -20°C. Prolonged exposure to this temperature can precipitate undesired salts.

12. Repeat Step 7.
13. Remove the supernatant.
14. Gently overlay the pellets with 200 µl of 80% ethanol.
15. Centrifuge at 14,000 rpm for 5 min.
16. Carefully remove the supernatant.
17. Air-dry the pellets for 5–10 min.
18. Dissolve the pellet in 5.5 µl of H₂O and store at -20°C.

These 5.5 µl samples of Rsa I-digested cDNA will serve as your **experimental driver cDNA** and your **control skeletal muscle driver cDNA**. In the next section, these samples will be ligated with adaptors to create your tester cDNAs for forward, control, and reverse (if applicable) subtractions.

19. Check your Rsa I-digested cDNA from Step IV.E.4 using agarose/EtBr gel electrophoresis, as described in Section V.B. Then, proceed to Section IV.F to finish preparing your experimental and control skeletal muscle **tester cDNAs**.

F. Protocol: Adaptor Ligation

Figure 3 shows the experimental flowchart for preparing adaptor-ligated tester cDNA. If you plan to perform differential screening of the subtracted library (discussed in detail in Section VI), you must perform subtractions in both forward and reverse directions for each tester/driver cDNA pair—so you will need to prepare tester cDNA corresponding to each of your poly A⁺ RNA samples.

General Considerations

- Forward subtraction** (Figure 3, Panel A) is designed to enrich for differentially expressed sequences present in poly A⁺ RNA sample 1 (cDNA 1, tester) but not poly A⁺ RNA sample 2 (cDNA 2, driver)—producing a subtracted cDNA population with sequences specific to sample 1.
- Reverse subtraction** (Figure 3, Panel B) uses cDNA 2 as tester and cDNA 1 as driver—producing a subtracted cDNA population with sequences specific to sample 2. Even if you are only interested in sequences specific to sample 1, the reverse-subtracted cDNA can be used for differential screening (Section VI).
- Control subtraction** (Figure 3, Panel C) should also be performed. In Step 2 (below), you will prepare tester cDNA for this control subtraction by mixing the control skeletal muscle cDNA with φX174/Hae III DNA.

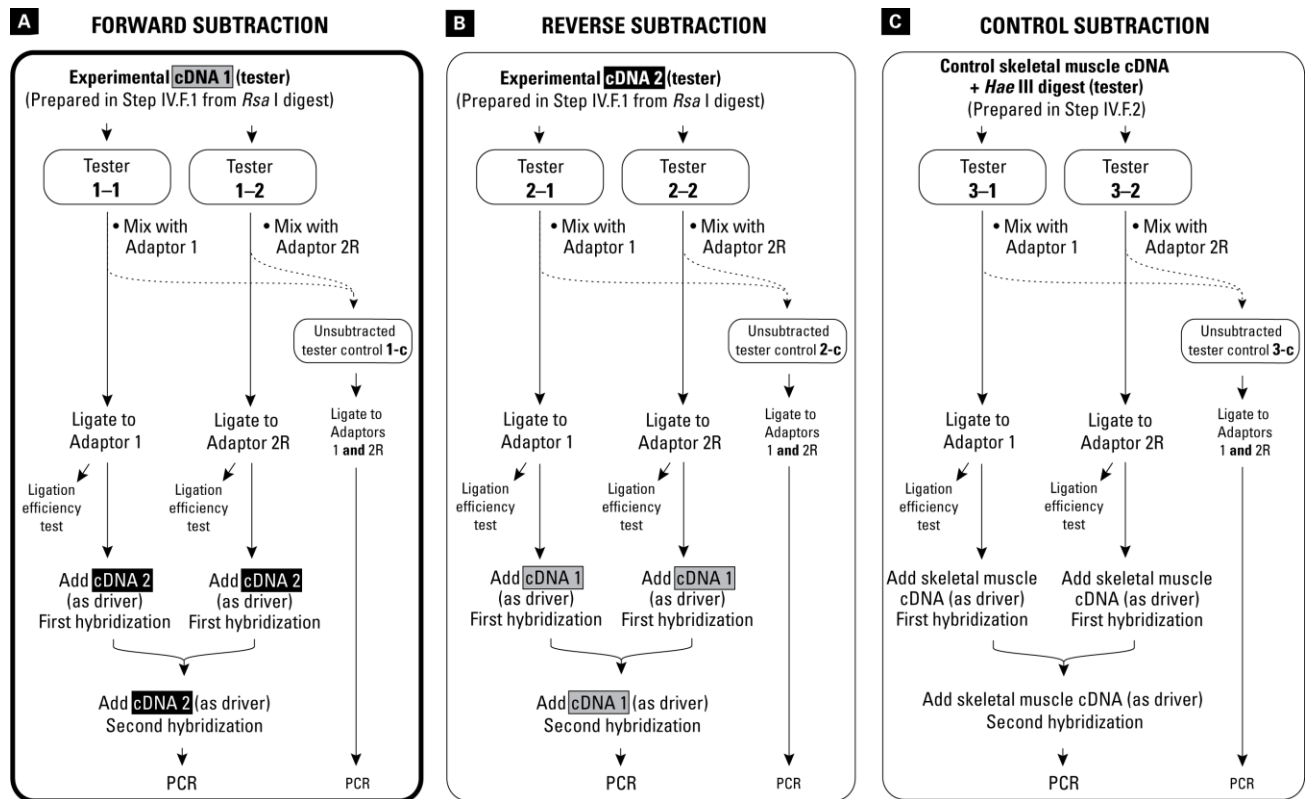


Figure 3. Preparing adaptor-ligated tester cDNAs for hybridization and PCR. Each tester cDNA (i.e., each different experimental cDNA and your control skeletal muscle tester cDNA) must be ligated to the appropriate adaptors as shown above. **Panel A.** The forward subtraction is your intended experiment. **Panel B.** A second subtraction in reverse (i.e., tester as driver, driver as tester) is required for differential screening of the subtracted cDNA library (Section VI). **Panel C.** Control subtraction with skeletal muscle cDNA.

Procedure for Adaptor Ligation

Three separate adaptor ligations (Figure 3) must be performed for each experimental tester cDNA and the control skeletal muscle tester cDNA:

IMPORTANT: Adaptors should not be ligated to the driver cDNA.

General Ligation Set-up

- Each cDNA is aliquoted into two separate tubes: one aliquot is ligated with Adaptor 1 (Tester 1-1, 2-1, and 3-1), and the second is ligated with Adaptor 2R (Tester 1-2, 2-2, and 3-2).
- After the ligation reactions are set up, portions of each tester tube are combined so that the cDNA is ligated with both adaptors (unsubtracted tester control 1-c, 2-c, and 3-c).
- Each unsubtracted tester control cDNA serves as a positive ligation control, and later as a negative subtraction control.

NOTE: Throughout the procedure, it is helpful to label tubes using the nomenclature described in this user manual. Labeling tubes of intermediate products with the appropriate step number in which they were created may prove helpful as well. Refer to Figure 3 to help you keep track of the multiple samples.

Ligation Protocol

1. Prepare your experimental tester cDNA 1 and tester cDNA 2:

- a. Dilute 1 µl of each Rsa I-digested experimental cDNA (Step IV.E.18) with 5 µl of sterile H₂O.

If you have used the SMARTer Pico PCR cDNA Synthesis Kit to prepare your cDNA, use the purified, Rsa I-digested cDNAs from the SMARTer Pico procedure for this dilution.

2. Prepare your control skeletal muscle tester cDNA:

- a. Dilute the φX174/Hae III Control DNA with sterile H₂O to a final concentration of 150 ng/ml.
- b. Mix 1 µl of control skeletal muscle cDNA (Step IV.E.18) with 5 µl of the diluted φX174/Hae III Control DNA (150 ng/ml).
 - This is your control skeletal muscle tester cDNA. It contains 0.2% Hae III-digested φX174 DNA; each fragment corresponds to about 0.02% of the total cDNA. After subtraction of the skeletal muscle tester cDNA against the skeletal muscle driver cDNA, the primary bands produced in the final PCR should correspond to these control fragments.
 - If you have used the SMARTer Pico PCR cDNA Synthesis Kit to prepare your cDNA, you should repeat Step 2 above using the mouse liver cDNA from the SMARTer Pico procedure (as described in the SMARTer Pico PCR cDNA Synthesis Kit User Manual at www.clontech.com/manuals). For the rest of the PCR-Select protocol, you should analyze the control mouse liver cDNA in parallel with the control skeletal muscle cDNA.

3. Ligate your tester cDNAs to the appropriate adaptors:

- a. Prepare a ligation Master Mix by combining the following reagents in a 0.5 ml microcentrifuge tube. To ensure that you have sufficient Master Mix, prepare enough for all ligations plus one additional reaction.

	<u>per rxn</u>
Sterile H ₂ O	3 µl
5X Ligation Buffer	2 µl
T4 DNA Ligase (400 units/µl)	1 µl

- b. For each experimental tester cDNA and for the control skeletal muscle tester cDNA, combine the reagents in Table 1 in the order shown in 0.5 ml microcentrifuge tubes. Pipet mixture up and down to mix thoroughly.

Table 1. Setting up the Ligation Reactions

(Repeat for each experimental tester cDNA & the control skeletal muscle tester cDNA)

	Tube Number	
	1 Tester 1-1*	2 Tester 1-2*
Diluted tester cDNA	2 µl	2 µl
Adaptor 1 (10 µM)	2 µl	—
Adaptor 2R (10 µM)	—	2 µl
Master Mix	6 µl	6 µl
Final volume	10 µl	10 µl

*Use the same setup for Tester 2-1 and 2-2, 3-1 and 3-2.

- c. In a fresh microcentrifuge tube, mix 2 µl of Tester 1-1 and 2 µl of Tester 1-2. After ligation is complete, this will be your unsubtracted tester control 1-c (see Figure 3). Do the same for each additional experimental tester cDNA and the control skeletal muscle tester cDNA. After ligation, approximately 1/3 of the cDNA molecules in each unsubtracted tester control tube will bear two different adaptors.
- d. Centrifuge briefly, and incubate at 16°C overnight.
- e. Add 1 µl of EDTA/Glycogen Mix to stop ligation reaction.
- f. Heat samples at 72°C for 5 min to inactivate the ligase.
- g. Briefly centrifuge the tubes. Your experimental and control skeletal muscle Adaptor-Ligated Tester cDNAs and unsubtracted tester controls are now complete.
- h. Remove 1 µl from each unsubtracted tester control (1-c, 2-c, 3-c) and dilute into 1 ml of H₂O. These samples will be used for PCR (Section IV.I).
- i. Store samples at -20°C.

G. Protocol: First Hybridization

Perform the ligation efficiency analysis in Section V.C. **before proceeding with the hybridizations described below.** If your ligation was not efficient, repeat the ligation step before proceeding any further.

IMPORTANT: Before you begin the hybridization, **allow the 4X Hybridization Buffer to warm up to room temperature for at least 15–20 min.** Verify that there is no visible pellet or precipitate before using the buffer. If necessary, heat the buffer at 37°C for ~10 min to dissolve any precipitate.

1. For each of the experimental and skeletal muscle subtractions, combine the reagents in Table 2 in 0.5 ml tubes in the order shown.

Table 2. Setting Up the First Hybridization

(Repeat for each experimental tester cDNA & the control skeletal muscle tester cDNA)

Component	Hybridization Sample	
	1 Tester 1-1*	2 Tester 1-2*
Rsa I-digested Driver cDNA (IV.E.18)	1.5 µl	1.5 µl
Adaptor 1-ligated Tester 1-1* (IV.F.3.i)	1.5 µl	—
Adaptor 2R-ligated Tester 1-2 (IV.F.3.i)	—	1.5 µl
4X Hybridization Buffer	1.0 µl	1.0 µl
Final volume	4.0 µl	4.0 µl

*Use the same setup for Tester 2-1 and 2-2, 3-1 and 3-2.

2. Overlay samples with one drop of mineral oil and centrifuge briefly.
3. Incubate samples at 98°C for 1.5 min in a thermal cycler.
4. Incubate samples at 68°C for 8 hr*

*Samples may hybridize for 6–12 hr. **Do not let the incubation exceed 12 hours.**

H. Protocol: Second Hybridization

IMPORTANT: Do not denature the primary hybridization samples at this stage. Also, do not remove the hybridization samples from the thermal cycler for longer than is necessary to add fresh driver.

Repeat the following steps for each experimental tester cDNA and for the control skeletal muscle cDNA.

1. Add the following reagents into a sterile tube:

	per rxn
Driver cDNA (Step IV.E.18)	1 µl
4X Hybridization Buffer	1 µl
Sterile H ₂ O	2 µl

2. Place 1 µl of this mixture in a 0.5 ml microcentrifuge tube and overlay it with 1 drop of mineral oil.
3. Incubate at 98°C for 1.5 min in a thermal cycler.

4. Remove the tube of freshly denatured driver from the thermal cycler. Use the following procedure to simultaneously mix the driver with hybridization samples 1 and 2 (prepared in Section IV.G; see Table 2). This ensures that the two hybridization samples mix together only in the presence of freshly denatured driver.
 - a. Set a micropipettor at 15 μ l.
 - b. Gently touch the pipette tip to the mineral oil/sample interface of the tube containing hybridization sample 2.
 - c. Carefully draw the entire sample partially into the pipette tip. Do not be concerned if a small amount of mineral oil is transferred with the sample.
 - d. Remove the pipette tip from the tube, and draw a small amount of air into the tip, creating a slight air space below the droplet of sample.
 - e. Repeat steps b–d with the tube containing the freshly denatured driver. The pipette tip should now contain both samples (hybridization sample 2 and denatured driver) separated by a small air pocket.
 - f. Transfer the entire mixture to the tube containing hybridization sample 1.
 - g. Mix by pipetting up and down.
5. Briefly centrifuge if necessary.
6. Incubate reaction at 68°C overnight.
7. Add 200 μ l of dilution buffer and mix by pipetting.
8. Heat at 68°C for 7 min in a thermal cycler.
9. Store at –20°C.

I. Protocol: PCR Amplification

A minimum of seven PCR reactions are recommended as described in Figure 3:

- 1) Forward-subtracted experimental cDNA
- 2) Unsubtracted tester control (1-c)
- 3) Reverse-subtracted experimental cDNA
- 4) Unsubtracted tester control for the reverse subtraction (2-c)
- 5) Subtracted control skeletal muscle cDNA
- 6) Unsubtracted tester control for the control subtraction (3-c)
- 7) PCR control-subtracted cDNA

The PCR control subtracted cDNA provides a positive PCR control and contains a successfully subtracted mixture of Hae III-digested ϕ X174 DNA. We recommend that you also perform a standard PCR control (i.e., the positive control template in the Advantage cDNA PCR Kit) to verify that your enzyme is performing efficiently.

PCR Amplification Procedure

1. Prepare the PCR templates:
 - a. Aliquot 1 µl of each diluted cDNA (i.e., each subtracted sample from Step IV.H.9 and the corresponding diluted unsubtracted tester control from Step IV.F.3.i) into an appropriately labeled tube.
 - b. Aliquot 1 µl of the PCR control subtracted cDNA into an appropriately labeled tube.
2. Prepare a Master Mix for all of the primary PCR tubes plus one additional tube. For each reaction planned, combine the reagents in Table 3 in the order shown:

Table 3. Preparation of the Primary PCR Master Mix

Reagent	Per Rxn	7-Rxn Mix*
Sterile H ₂ O	19.5 µl	156.0 µl
10X PCR reaction buffer	2.5 µl	20.0 µl
dNTP Mix (10 mM)	0.5 µl	4.0 µl
PCR Primer 1 (10 µM)	1.0 µl	8.0 µl
50X Advantage cDNA Polymerase Mix	0.5 µl	4.0 µl
Total volume	24.0 µl	192.0 µl

* For each additional experimental cDNA, prepare Master Mix for one additional reaction.

3. Mix well by vortexing, and briefly centrifuge the tube.
4. Aliquot 24 µl of Master Mix into each of the reaction tubes prepared in Step 1.
5. Overlay with 50 µl of mineral oil.
6. Incubate the reaction mix at 75°C for 5 min in a thermal cycler to extend the adaptors. (Do not remove the samples from the thermal cycler.)

NOTE: This step “fills in” the missing strand of the adaptors (see Figure 2), thus creating binding sites for the PCR primers.

7. Immediately commence thermal cycling:

Cycle Parameters	
Cold Lid	Hot Lid
27 cycles: <ul style="list-style-type: none"> • 94°C for 30 sec • 66°C for 30 sec • 72°C for 1.5 min 	27 cycles: <ul style="list-style-type: none"> • 94°C for 25 sec • 94°C for 10 sec • 66°C for 30 sec • 72°C for 1.5 min

8. Analyze 8 µl from each tube on a 2.0% agarose/EtBr gel run in 1X TAE buffer. (See Section V.D for expected results.) Alternatively, you can set these 8 µl aliquots aside and run them on the same gel used to analyze the secondary PCR products (Step 16).
9. Dilute 3 µl of each primary PCR mixture in 27 µl of H₂O. [If applicable: this diluted primary PCR product is used in the PCR-Select Differential Screening Kit procedure.]
10. Aliquot 1 µl of each diluted primary PCR product mixture from Step 9 into an appropriately labeled tube.

11. Prepare Master Mix for the secondary PCR reactions plus one additional reaction by combining the reagents in Table 4 in the order shown:

Table 4. Preparation of the Secondary PCR Master Mix

Reagent	Per Rxn	7-Rxn Mix*
Sterile H ₂ O	18.5 µl	156.0 µl
10X PCR reaction buffer	2.5 µl	20.0 µl
Nested PCR primer 1 (10 µM)	1.0 µl	8.0 µl
Nested PCR primer 2R (10 µM)	1.0 µl	8.0 µl
dNTP Mix (10 mM)	0.5 µl	4.0 µl
50X Advantage cDNA Polymerase Mix	0.5 µl	4.0 µl
Total volume	24.0 µl	192.0 µl

* For each additional experimental cDNA, prepare Master Mix for one additional reaction.

12. Mix well by vortexing, and briefly centrifuge.
13. Aliquot 24 µl of Master Mix into each reaction from Step 10.
14. Overlay with 1 drop of mineral oil.
15. Immediately commence thermal cycling:

Cycle Parameters	
Cold Lid	Hot Lid
10–12 cycles: <ul style="list-style-type: none"> • 94°C for 30 sec • 68°C for 30 sec • 72°C for 1.5 min 	10–12 cycles: <ul style="list-style-type: none"> • 94°C for 10 sec • 68°C for 30 sec • 72°C for 1.5 min

16. Analyze 8 µl from each reaction on a 2.0% agarose/EtBr gel run in 1X TAE buffer. (See Section V.D for expected results.)
17. Store reaction products at –20°C.

- The PCR mixture is now enriched for differentially expressed cDNAs. In addition, differentially expressed transcripts that varied in abundance in the original mRNA sample should now be present in roughly equal proportions. Refer to Sections V.D and V.E. Figure 6 shows the results of a successful control subtraction experiment with cDNA made from the skeletal muscle poly A⁺ RNA. We strongly recommend that you perform a subtraction efficiency test as shown in Figures 7 and 8.
- The uncloned subtracted mixture is an ideal hybridization probe for screening libraries of genomic DNA, full-length cDNA, YAC, BAC, or cosmid clones (Diatchenko *et al.*, 1996). For all other applications, you should clone the products to make a subtracted cDNA library.
- For further analysis of your subtracted library, several options are available:
 - **Differential screening**
Our PCR-Select Differential Screening Kit (Cat. No. 637403) contains the necessary reagents for differential screening, along with controls. For more information, see Section VI and the PCR-Select Differential Screening Kit User Manual at www.clontech.com/manuals
 - **Northern analysis**
 - **Virtual Northern**s

V. Analysis of Results & Troubleshooting Guide

A. Analysis of ds cDNA Synthesis Products

Troubleshooting of dsDNA Synthesis

- If agarose gel analysis indicates that the yield of your experimental ds cDNA is low in comparison with the ds cDNA produced from the skeletal muscle poly A⁺ RNA, but the size distribution is similar, you may still use your cDNA. However, it is highly likely that you may have lost some low-abundance, differentially-expressed sequences. Alternatively, you may repeat the synthesis using a higher concentration of poly A⁺ RNA for first-strand cDNA synthesis.
- The optimal concentration of poly A⁺ RNA for first-strand cDNA synthesis is 50–200 µg/ml. If you use a lower concentration of RNA, the size distribution of cDNA products synthesized may be reduced.

B. Analysis of Rsa I Digestion

Electrophorese 2.5 µl of undigested, ds cDNA (from Section IV.D) and 5 µl of Rsa I-digested cDNA (from Section IV.E) on a 1% agarose/EtBr gel in 1X TAE buffer side-by-side.

- cDNA derived from poly A⁺ RNA appears as a smear from 0.5–10 kb.
- Bright bands correspond to abundant mRNAs or rRNAs. (Size distribution may be only 0.5–3 kb for some RNA samples from nonmammalian species.)
- After Rsa I digestion, the average cDNA size is smaller (0.1–2 kb compared to 0.5–10 kb). Typical results are shown in Figure 4. If the size distribution of your sample and/or control cDNA is not reduced after Rsa I digestion, repeat the phenol/chloroform extraction, ethanol precipitation, and digestion steps.
- **[Optional]** To determine if a sample is completely digested, remove a small sample of DNA at 60 and 80 min. Compare the samples on an agarose gel. If the DNA size distribution for both samples is identical, digestion has progressed to completion.

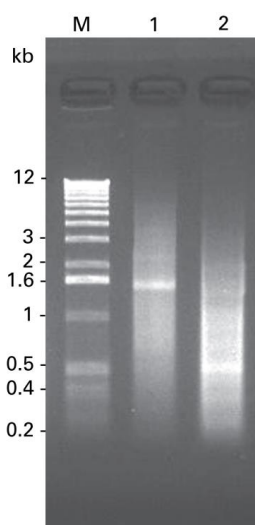


Figure 4. Positive control skeletal muscle ds cDNA before (Lane 1) and after (Lane 2) Rsa I digestion. cDNA was synthesized as described in the protocol using the human skeletal muscle control poly A⁺ RNA included in the kit. Lane M: DNA size markers.

C. Analysis of Ligation

We recommend that you perform the following PCR experiment to verify that at least 25% of the cDNAs have adaptors on both ends. This experiment is designed to amplify fragments that span the adaptor/cDNA junctions of Testers 1-1 and 1-2. (See Section IV.F.)

- You should also perform this analysis on your adaptor-ligated control skeletal muscle cDNA (3-1 and 3-2) and, if doing the reverse subtraction, with your second experimental tester cDNA (2-1 and 2-2).
- The G3PDH primers in this control experiment will work for human, mouse, and rat genes. For other species, you will need to design suitable primers.

Ligation Analysis Procedure

1. Dilute 1 µl of each ligated cDNA from Sec. IV.F (e.g., the Testers 1-1 and 1-2) into 200 µl of H₂O.
2. Combine the reagents in Table 5 in four separate tubes:

Table 5. Setting Up the Ligation Analysis

(Repeat for each experimental tester cDNA & the control skeletal muscle cDNA)

Component	Tube (µl)			
	1	2	3	4
Tester 1-1* (ligated to Adaptor 1)	1	1	—	—
Tester 1-2* (ligated to Adaptor 2R)	—	—	1	1
G3PDH 3' Primer (10 µM)	1	1	1	1
G3PDH 5' Primer (10 µM)	—	1	—	1
PCR Primer 1 (10 µM)	1	—	1	—
Total volume	3	3	3	3

* Use the same set-up for Tester 2-1 and 2-2, 3-1 and 3-2.

3. Prepare a Master Mix for all of the reaction tubes plus one additional tube. For each reaction planned, combine the reagents in Table 6 in the order shown:

Table 6. Preparation of the Ligation Analysis PCR Master Mix

Component	Per Rxn	4-Rxn Mix
Sterile H ₂ O	18.5 µl	92.5 µl
10X PCR reaction buffer	2.5 µl	12.5 µl
dNTP Mix (10 mM)	0.5 µl	2.5 µl
50X Advantage cDNA Polymerase Mix	0.5 µl	2.5 µl
Total volume	22.0 µl	110.0 µl

4. Mix well by vortexing and briefly centrifuging.
5. Aliquot 22 µl of Master Mix into each of the reactions from Step 2.
6. Mix well by vortexing and briefly centrifuging.
7. Overlay with 50 µl of mineral oil.
8. Incubate the reaction mix at 75°C for 5 min in a thermal cycler to extend the adaptors. (Do not remove the samples from the thermal cycler.)

NOTE: This step “fills in” the missing strand of the adaptors (see Figure 2), thus creating binding sites for the PCR primers.

9. Immediately commence thermal cycling:

Cycle Parameters	
Cold Lid	Hot Lid
20 cycles: <ul style="list-style-type: none"> • 94°C for 30 sec • 65°C for 30 sec • 68°C for 2.5 min 	20 cycles: <ul style="list-style-type: none"> • 94°C for 30 sec • 94°C for 10 sec • 65°C for 30 sec • 68°C for 2.5 min

10. Analyze 5 µl from each reaction on a 2.0% agarose/EtBr gel run in 1X TAE buffer.

- **Typical results are shown in Figure 5. If you cannot detect a product after 20 cycles**, perform 5 additional cycles, and analyze by gel electrophoresis. Additional PCR cycles may be necessary as G3PDH expression varies among tissues—its abundance in skeletal muscle is relatively high. As shown in Figure 5, the PCR product using one gene-specific primer (G3PDH 3' Primer) and PCR Primer 1 should be about the same intensity as the PCR product amplified using two gene-specific primers (G3PDH 3' and 5' Primers). If the band intensity for these PCR products differs by more than 4-fold, your ligation was less than 25% complete and will significantly reduce subtraction efficiency.
- **If you are working with mouse or rat cDNA**, the PCR product amplified using the G3PDH 3' Primer and PCR Primer 1 will be ~1.2 kb instead of 0.75 kb for human cDNA (rat and mouse G3PDH cDNAs lack an Rsa I restriction site). However, if you are working with human cDNA (which does contain the Rsa I site), and you observe this 1.2-kb band along with a band of the expected size, your cDNA is not fully digested. If there is a significant amount of this undigested product, you should repeat the Rsa I digestion.
- **If the above analysis shows poor ligation efficiency**, it is likely that either your cDNA was contaminated by undesired salt during a precipitation step, or second-strand synthesis was inefficient. Therefore, we recommend that you repeat the PCR-Select procedure starting with First-Strand cDNA Synthesis (Section IV.C).
- **Alternatively, if you have an insufficient quantity of RNA to resynthesize cDNA**, you can reprecipitate the remaining aliquots of each Rsa I-digested experimental and control cDNA (you should have 4.5 µl remaining from Step IV.E.19). Add 2.5 µl of 4 M NH₄OAc and 20 µl of 95% ethanol to each cDNA sample and follow the procedure of Section IV.E from Steps 12–19 before repeating the adaptor ligation procedure. We do not recommend reprecipitation as a primary troubleshooting solution for adaptor ligation failure because the recovery of cDNA may be inefficient, resulting in a low subtraction efficiency.

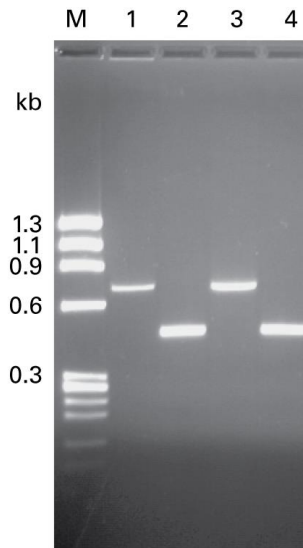


Figure 5. Typical results of ligation efficiency analysis. The results shown here are for human samples; if you are working with mouse or rat samples, the PCR product amplified using the G3PDH 3' Primer and PCR Primer 1 (Lane 3) will be ~1.2 kb instead of 0.75 kb. Lane 1: PCR products using Tester 1-1 (Adaptor 1-ligated) as the template and the G3PDH 3' Primer and PCR Primer 1. Lane 2: PCR products using Tester 1-1 (Adaptor 1-ligated) as the template, and the G3PDH 3' and 5' Primers. Lane 3: PCR products using Tester 1-2 (Adaptor 2R-ligated) as the template, and the G3PDH 3' Primer and PCR Primer 1. Lane 4: PCR products using Tester 1-2 (Adaptor 2R-ligated) as the template, and the G3PDH 3' and 5' Primers. 2% agarose/EtBr gel. Lane M: ϕ X174 DNA/Hae III digest size markers.

D. Analysis of PCR Products

1. Agarose/EtBr Gel Electrophoresis of Primary PCR

Perform your primary PCR side-by-side with the PCR control subtracted cDNA. With the PCR control subtracted cDNA, the major bands appearing after 27 cycles should correspond to the ϕ X174/Hae III fragments. This result should look similar to the skeletal muscle subtraction you performed; however, the correct ϕ X174/Hae III bands may appear only after secondary PCR. The experimental primary PCR subtraction products usually appear as a smear from 0.2–2 kb, with or without some distinct bands.

- a. **If you cannot see any products after 27 cycles**, use 3 additional cycles, and analyze by gel electrophoresis.
- b. **If you cannot detect PCR products in the subtracted or unsubtracted (unsubtracted tester control 1-c) samples or the PCR control subtracted mixture**, you must verify that your polymerase is working. If the problem is not with your polymerase mix, try optimizing the PCR cycling parameters in Step IV.I.7 by decreasing the annealing and extension temperature in small increments—each degree lower can dramatically increase the background. A starting point is to reduce the annealing temperature from 66°C to 64°C and the extension temperature from 72°C to 71°C.
- c. **If you can detect PCR products in the unsubtracted (unsubtracted tester control 1-c) samples, but not in the subtracted sample**, perform additional cycles of secondary PCR.

2. Agarose/EtBr Gel Analysis of Secondary PCR

The patterns of secondary PCR products from the PCR Control Subtracted cDNA and from your skeletal muscle subtraction should resemble Figure 6. A few additional bands may appear. The experimental subtracted samples usually appear as smears with or without a number of distinct bands.

- a. **If you do not observe ϕ X174/Hae III bands in the PCR control subtracted mixture**, you must optimize the PCR conditions.
- b. **If you can clearly see ϕ X174/Hae III bands in your unsubtracted skeletal muscle control**, it is likely that either the yield of your cDNA synthesis is very low, or you lost a majority of your skeletal muscle cDNA during phenol:chloroform extraction or ethanol precipitation.
- c. **If you obtain the expected ϕ X174/Hae III bands in the PCR control subtracted mixture, but not in your skeletal muscle control subtraction (e.g., smear or random size bands)**, it is likely that your subtraction was not optimal. One of the most likely explanations is poor ligation efficiency. For troubleshooting, see Section V.C.
- d. **If the ligation efficiency is high**, verify your protocol and repeat the subtraction. Problems during hybridization are uncommon.
- e. **If you cannot see a product after 12 cycles**, use 3 additional cycles, and analyze by gel electrophoresis. Add cycles sparingly as too many cycles can increase background.
- f. **In a successful subtraction**, the banding pattern of your unsubtracted cDNA ligated with both adaptors (unsubtracted tester control 1-c) should be different from the banding pattern of your experimental subtracted DNA samples (Figure 6).

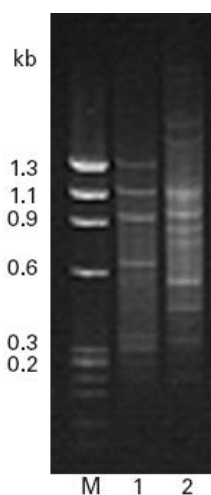


Figure 6. Typical results of control skeletal muscle subtraction analysis. The secondary PCR product of the subtracted skeletal muscle sample contains mostly DNA fragments corresponding to the ϕ X174/Hae III digest. The adaptor sequences on both ends of DNA fragments cause the mobility shift of these PCR products in comparison with original, digested ϕ X174 DNA. Lane M: ϕ X174 DNA/Hae III digest size markers. Lane 1: Secondary PCR products of subtracted skeletal muscle tester cDNA with 0.2% ϕ X174/Hae III-digested DNA. Lane 2: Secondary PCR products of unsubtracted skeletal muscle tester cDNA ligated with both Adaptors 1 and 2R (generated in Section IV.F) and containing 0.2% ϕ X174/Hae III-digested DNA. Samples are electrophoresed on a 2% agarose/EtBr gel.

E. PCR Analysis of Subtraction Efficiency

Either PCR (this section) or hybridization analysis (Section V.F) can be used to estimate the efficiency of subtraction by comparing the abundance of known cDNAs before and after subtraction. Ideally this is done with both a non-differentially expressed gene (e.g., a housekeeping gene), and with a gene known to be differentially expressed between the two RNA sources being compared. PCR provides a quicker test than hybridization analysis.

General Considerations

- **The test described below uses the G3PDH primers provided with the kit to confirm the reduced relative abundance of G3PDH** following the PCR-Select procedure. Note that these G3PDH primers can only be used for human, mouse, and rat genes. For other species, you will need to design suitable primers.
- **Not all housekeeping gene transcripts are subtracted evenly.** Although G3PDH is subtracted very efficiently in most tissues and cell lines, there are some exceptions, including skeletal muscle and heart. For this reason, we do not recommend the use of G3PDH abundance to analyze subtraction in the skeletal muscle control. Most other housekeeping genes are subtracted very efficiently from skeletal muscle and can therefore be used. In general, if the abundance of G3PDH did not decrease significantly after subtraction, you should check the abundance of other housekeeping genes (such as α -tubulin). However, in the control skeletal muscle subtraction experiment, the agarose gel banding pattern of the ϕ X174/Hae III digest (Figure 6, Lane 2) has already indicated whether or not subtraction was successful.
- **In certain instances a particular housekeeping gene is present at different levels in tester and driver poly A⁺ RNA.** If the concentration of G3PDH message is even 2-fold higher in the tester sample, G3PDH will not be efficiently subtracted out. If you perform subtraction in both directions (see Section IV.F) and have unsubtracted tester control for both the subtraction and the reverse subtraction, the PCR analysis of subtraction efficiency will indicate if there is any difference in G3PDH abundance in the two cDNA samples being compared. If this is the case, choose another housekeeping gene as a control for subtraction efficiency.
- **Clontech offers a number of RT-PCR Control Amplimer Sets for housekeeping genes** that can be used as positive controls for your studies. These include human, mouse, and rat Control Amplimer Sets for β -actin and G3PDH.

Procedure for PCR Analysis of Subtraction Efficiency

1. Dilute the subtracted and unsubtracted (unsubtracted tester control 1-c and 2-c) secondary PCR products 10-fold in H₂O. The concentration of subtracted and unsubtracted product should be roughly equal.
2. Combine the following reagents in 0.5 ml microcentrifuge tubes in the order shown:

	Rxn 1	Rxn 2
Diluted subtracted cDNA (2° PCR product)	1.0 μ l	—
Diluted unsubtracted tester control 1-c (2° PCR product)	—	1.0 μ l
G3PDH 3' Primer (10 μ M)	1.2 μ l	1.2 μ l
G3PDH 5' Primer (10 μ M)	1.2 μ l	1.2 μ l
sterile H ₂ O	22.4 μ l	22.4 μ l
10X PCR reaction buffer	3.0 μ l	3.0 μ l
dNTP Mix (10 mM each)	0.6 μ l	0.6 μ l
50X Advantage cDNA Polymerase Mix	0.6 μ l	0.6 μ l
Total volume	30.0 μl	30.0 μl

